

FIG. 1


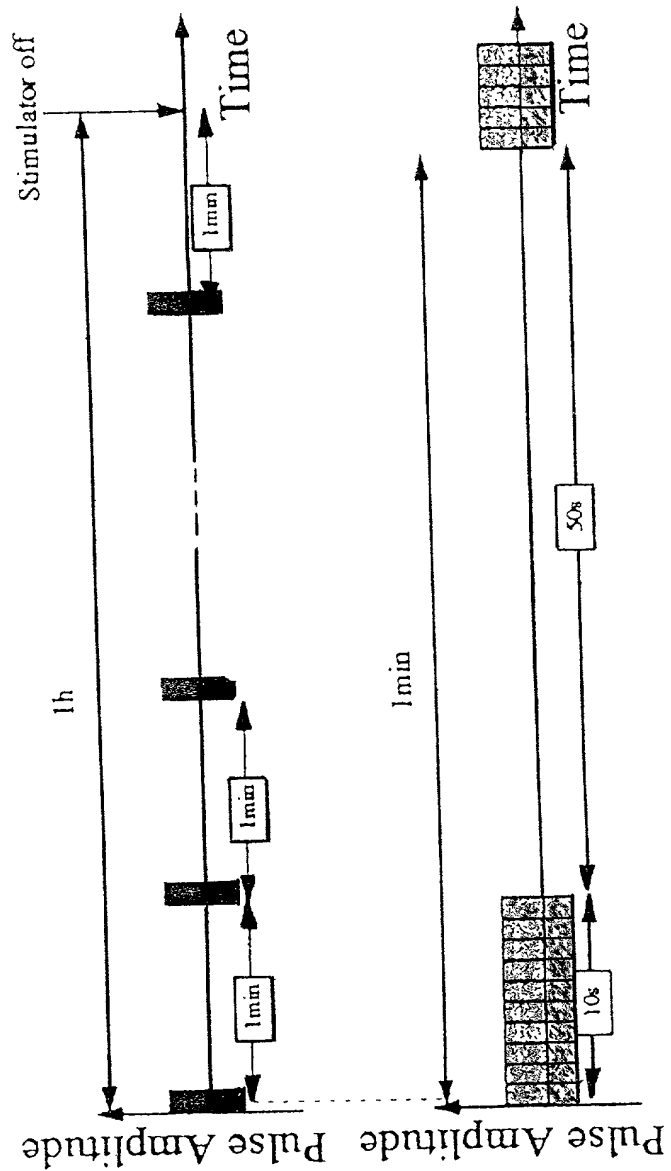


FIG. 2

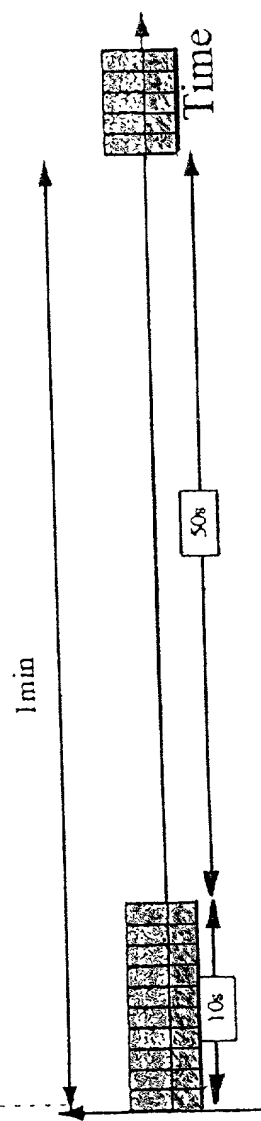

EEIG.3

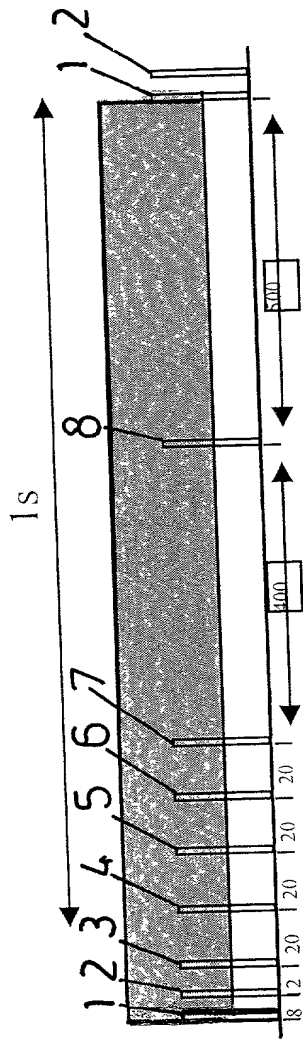


FIG. 4

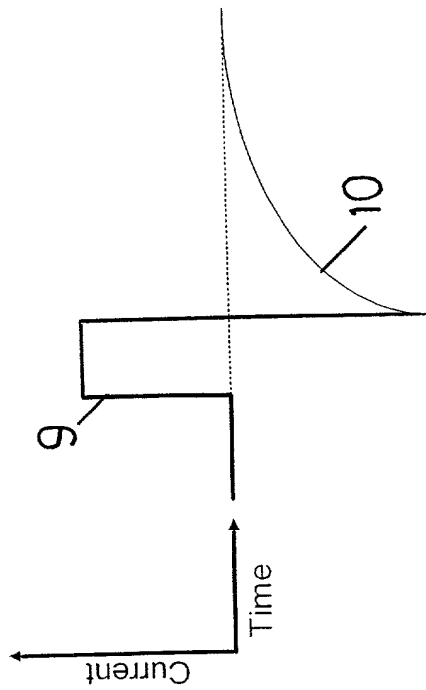


FIG. 5

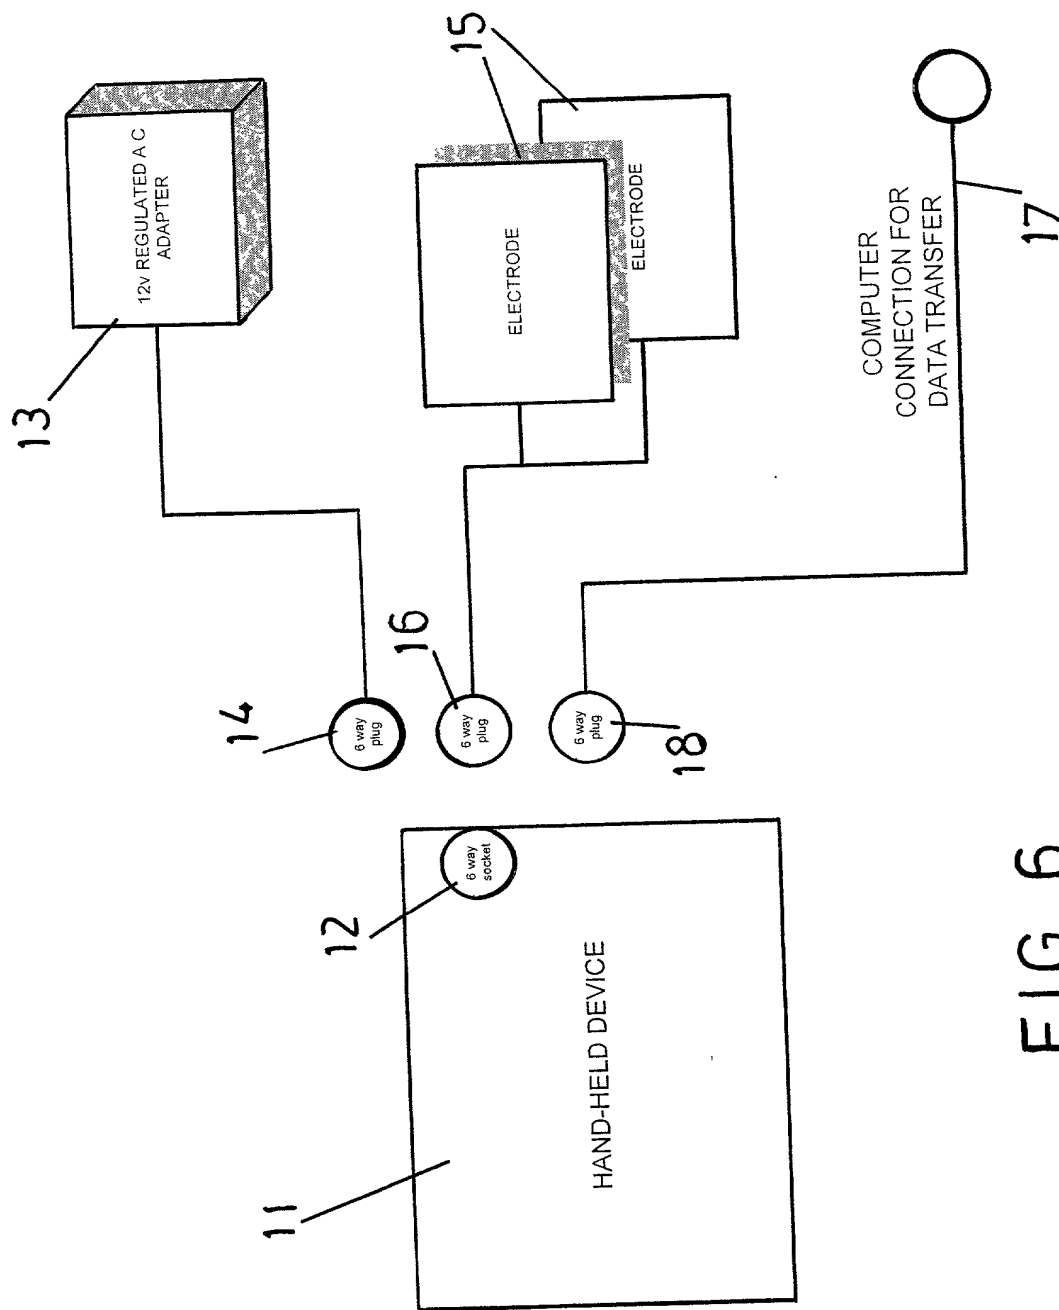


FIG. 6

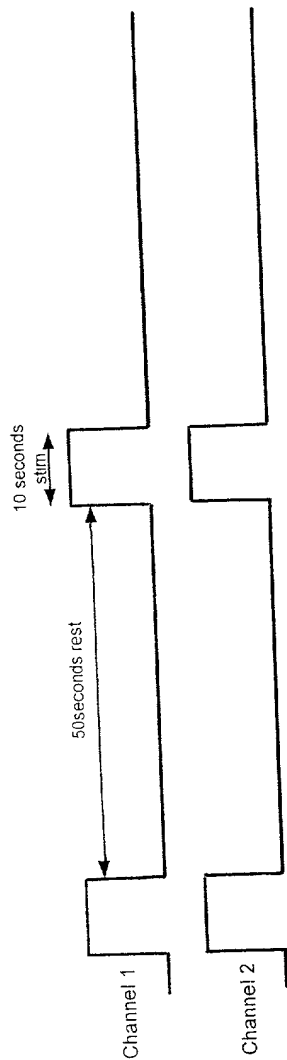


FIG. 7

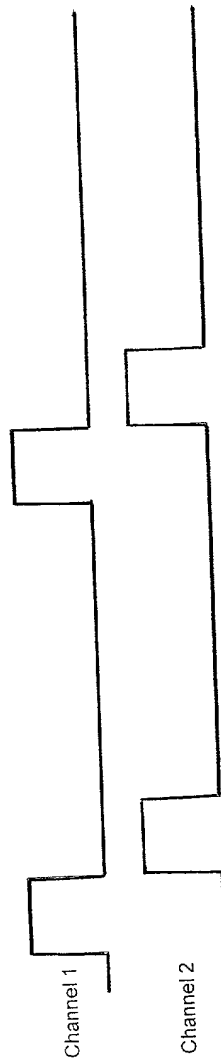


FIG. 8

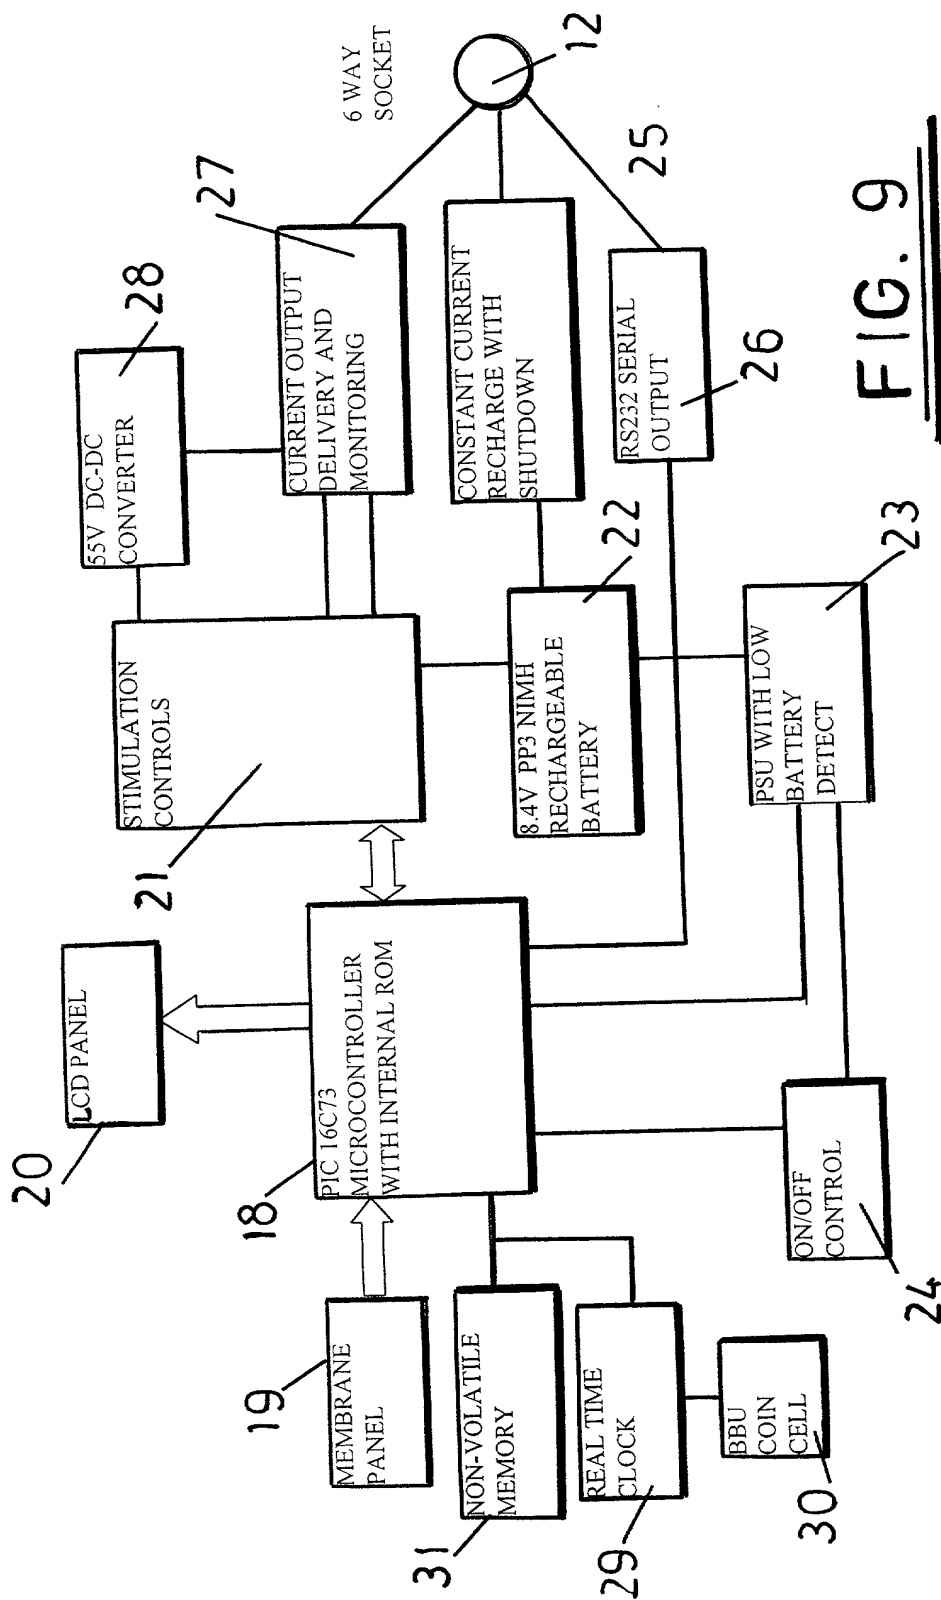


FIG. 9

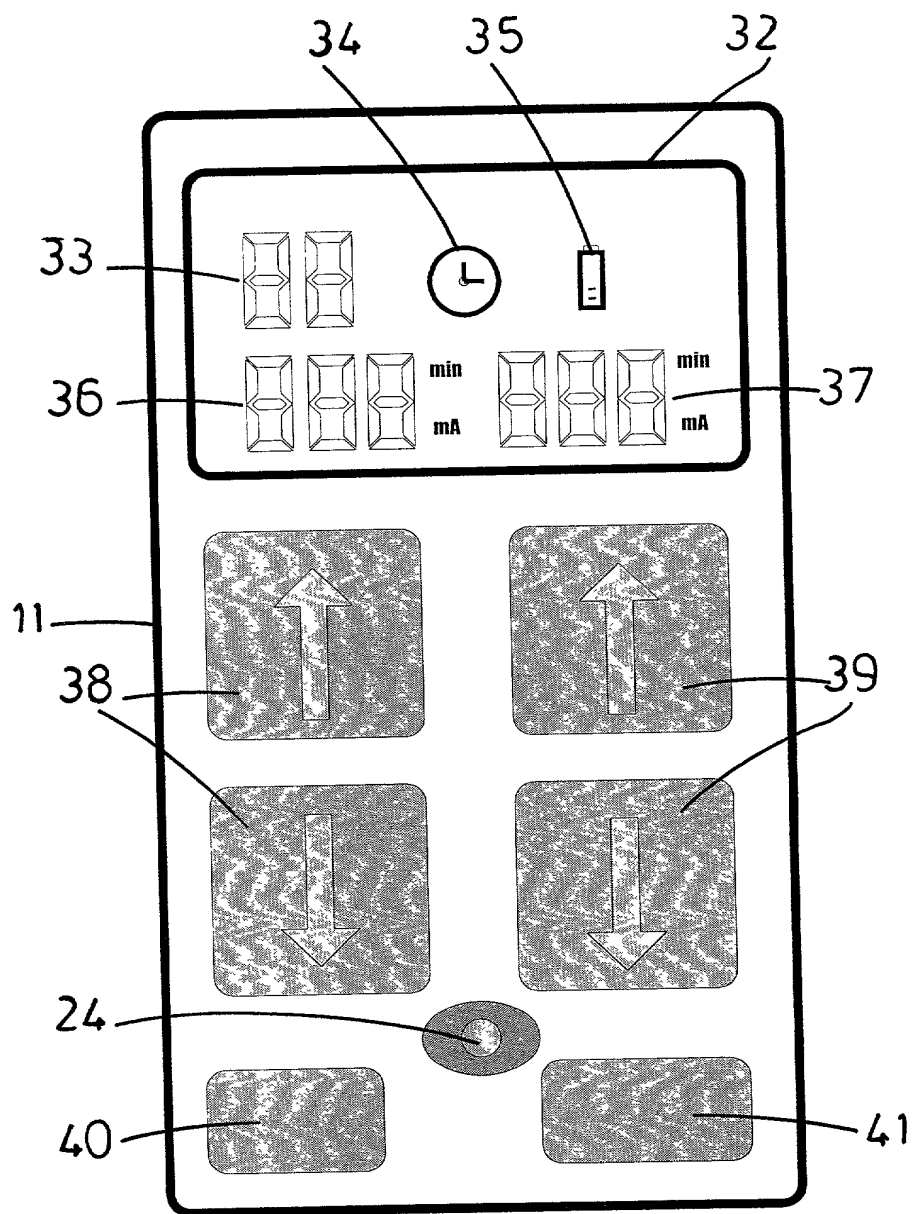


FIG. 10

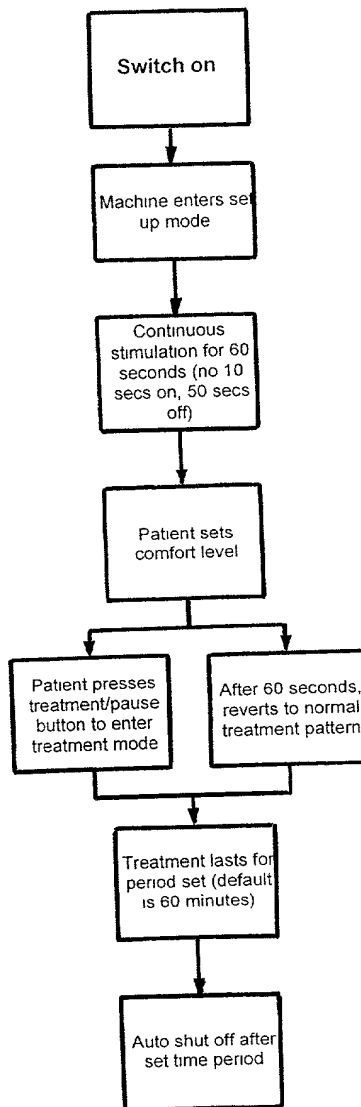


FIG. 11

Pause treatment

Press Treatment /
Pause button

To restart treatment

Press Treatment /
Pause button

```
graph TD; A[Press up or down keys to adjust during stimulation or rest phase] --> B[New intensity level is experienced during next stim phase]
```

Press up or down keys to adjust during stimulation or rest phase

New intensity level is experienced during next stim phase

FIG. 13

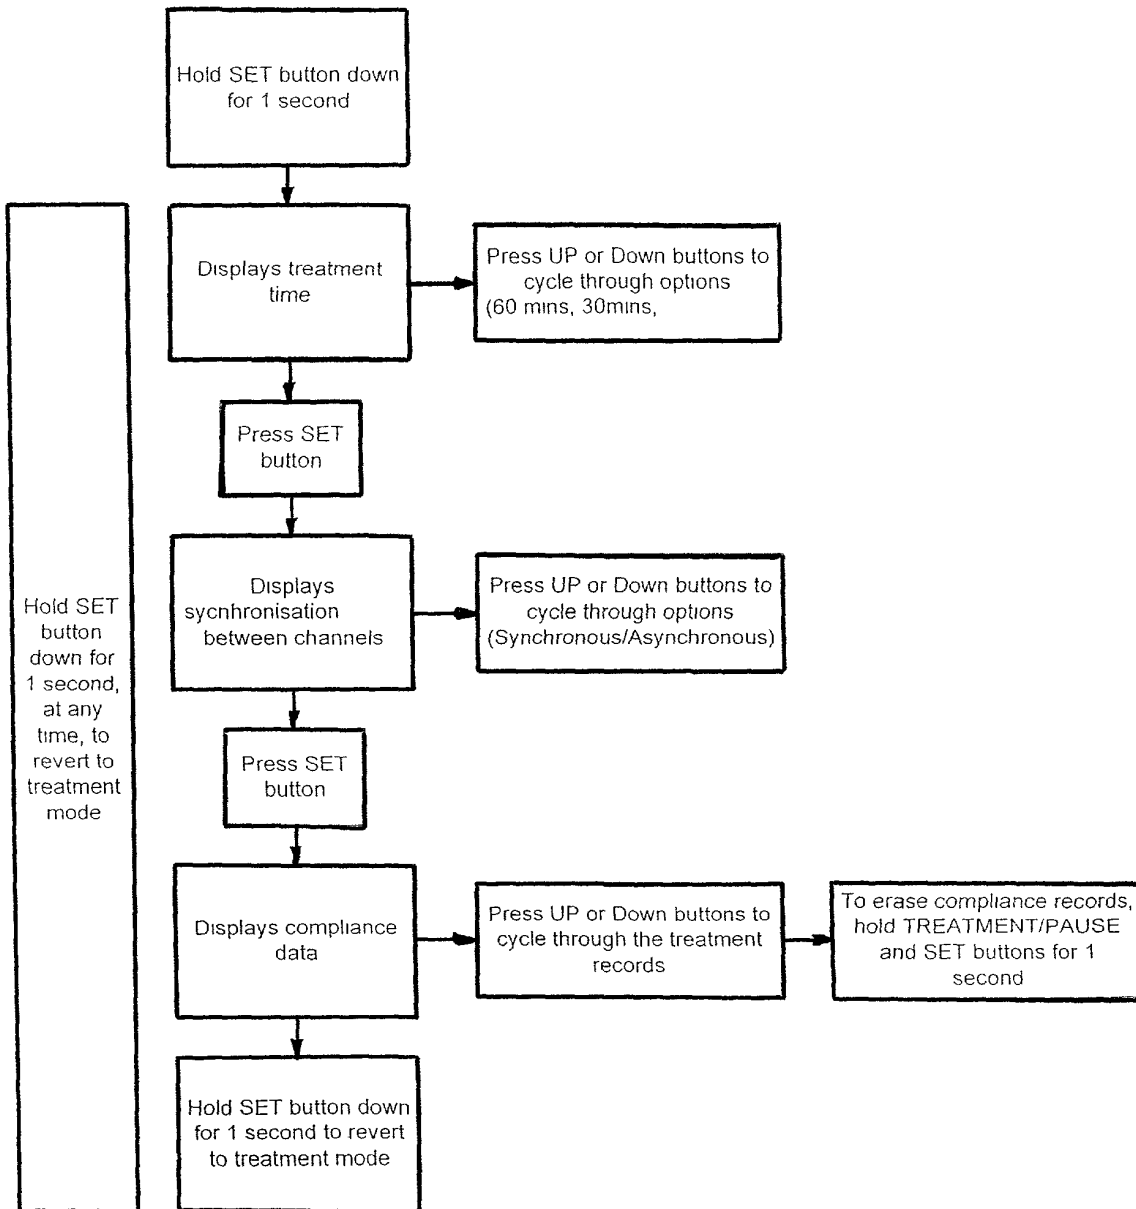


FIG.14

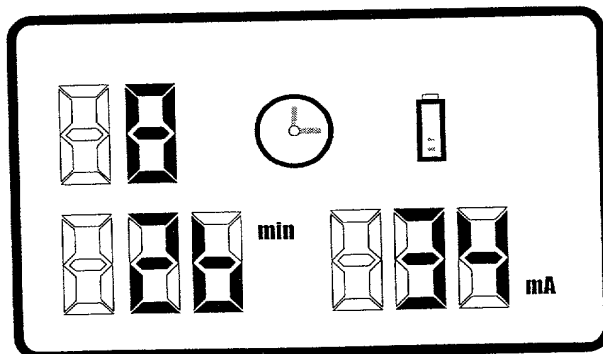
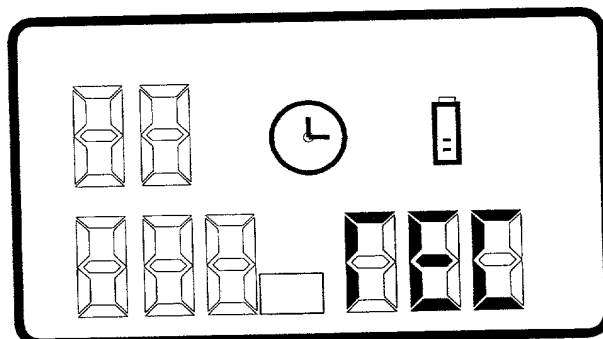
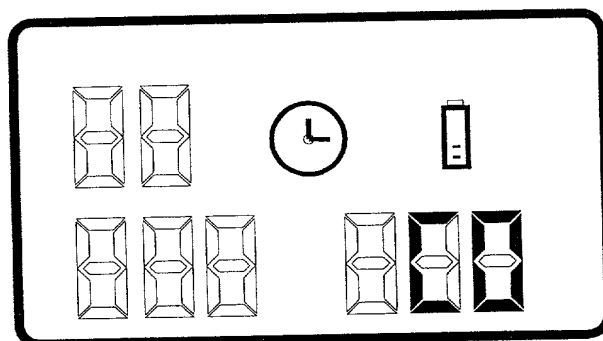
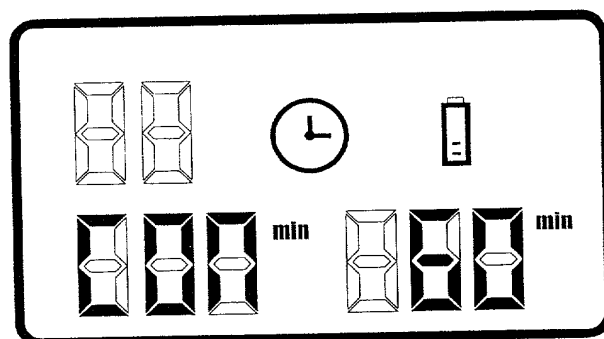


FIG. 15

00043297-100401

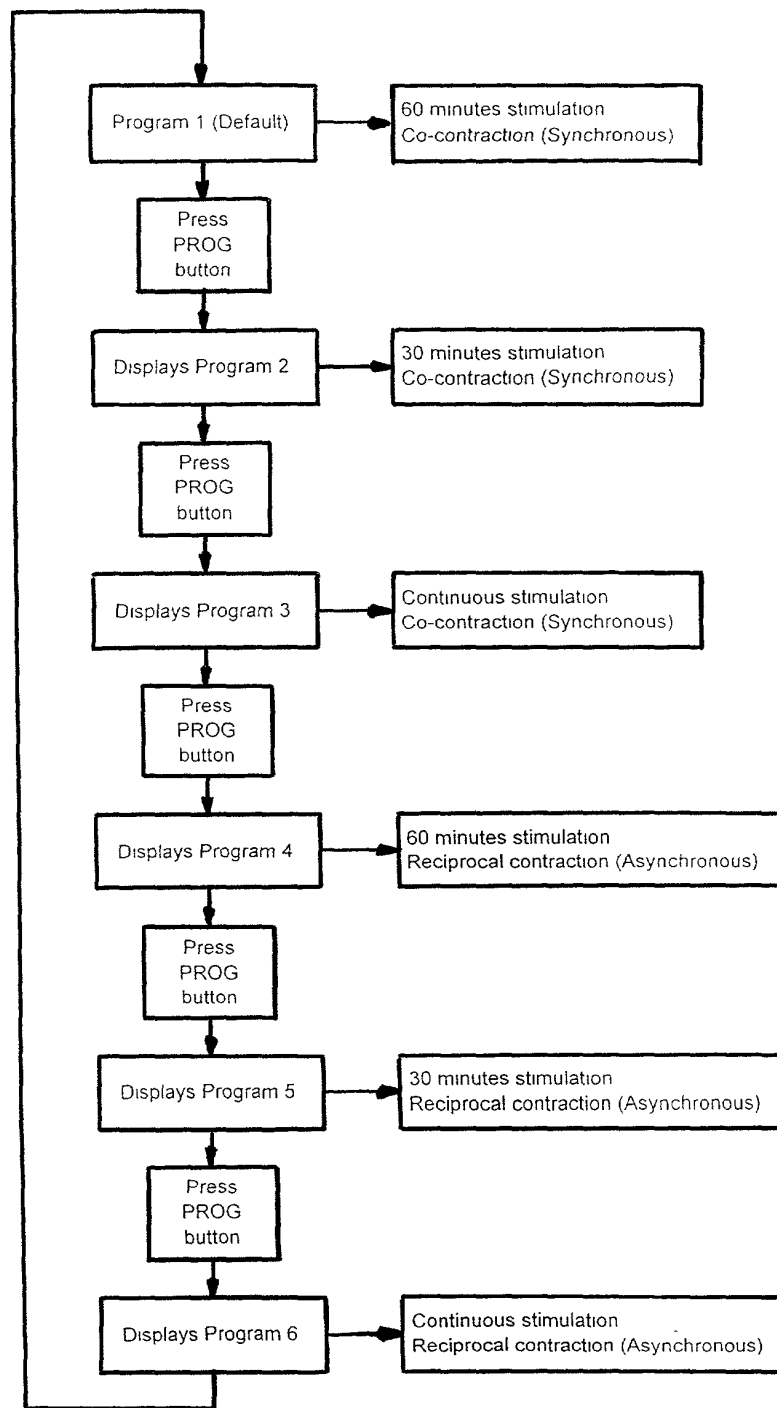


FIG.16

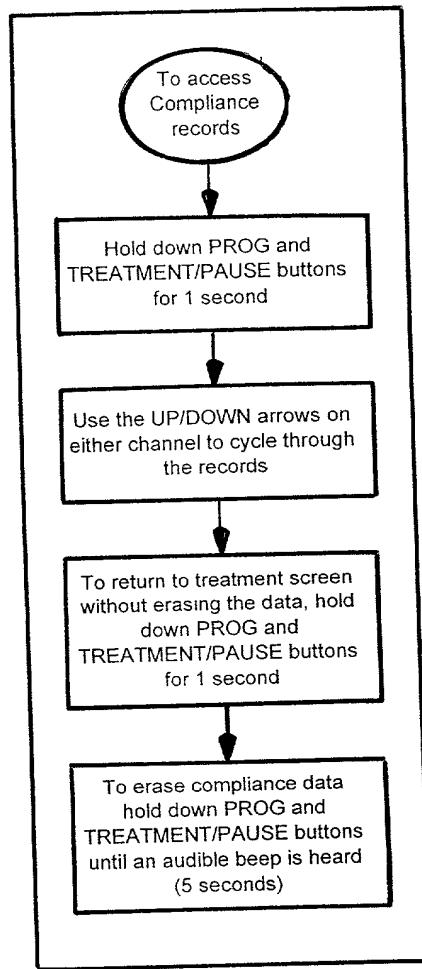


FIG. 17